



SGS

EU Type Examination Certificate Number: **0120/SGS0278**

ORNO-LOGISTIC Sp. Z O.O

Katowicka 134 43-190
Mikolow
Poland

Instrument Identification:
OR-WE-513, OR-WE-516, OR-WE-517

Polyphase, Active Import/Export (kWh), Electricity Meter

Instrument Traceable Number
0120/SGS0278

has been assessed and certified as meeting the requirements of

EU Directive 2014/32/EU

on Measuring Instruments Annex II, Module B

It is certified that the manufacturer's technical design and specimen for the above instrument has been examined and, based on the evidence submitted, it is considered that the instrument conforms to the requirements of Annex V of EU Directive 2014/32/EU

This certificate must be used in conjunction with a certificate covering the product verification as required in Annex II, Module D or Annex II, Module F

This certificate is valid until 14th March 2027
Issue 1

Certification is based on report number(s) SHES151200818401 Dated 17th March 2017
EMA234429/1
EMA238069/1

Authorised Signature

SGS United Kingdom Limited, Notified Body 0120
Unit 202B Worle Parkway, Weston-super-Mare, BS22 6WA, UK
t +44 (0)1934 522917 f +44 (0)1934 522137 www.sgs.com

SGS United Kingdom Ltd, Units 12A & 12B, South Industrial Estate, Bowburn, Durham, DH6 5AD, UK
t +44 (0)191 377 2000 f +44 (0)191 377 2020 www.sgs.com



This document is issued, on the Client's behalf, by the Company under its General Conditions of Service printed overleaf. The Client's attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein.

Any other holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Clients instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents.

MID-B-06F Rev 10

Page 1 of 9

EU Type Examination Cert.


SGSPAPER
18103187



1. Technical Data

Manufacturer	ORNO-LOGISTIC Sp. Z O.O.
Meter Types	OR-WE-513 OR-WE-516 OR-WE-517
Voltage Rating (U_n)	3x230/400V
Current Rating ($I_{min} - I_{ref} (I_{max})$)	0.25-5(30)A, 0.25-5(32)A, 0.25-5(40)A, 0.25-5(45)A, 0.25-5(50)A, 0.25-5(80)A,
Frequency (F_n)	50Hz
Active Accuracy Class (kWh)	A or B (kWh)
Type of circuit	3P4W
Temperature Range	-25°C to +55°C
Software/ Firmware Version No's	OR-WE-513: V1.01 OR-WE-516: V1.01 OR-WE-517: V1.01
Checksum	91E4
Identification Location	LCD & Nameplate
Bill Of Materials Numbers	OR-WE-513: D519032 OR-WE-516: D519033 OR-WE-517: D519024
IP Rating	IP51
Insulation Protective Class	Class II
LED Pulse Constant	1000imp/ kWh
Impulse Voltage Rating	6kV
AC Voltage Rating	4kV
Main Cover Sealing Type	Wire & Crimp
Integrity of meter	Inaccessible without breaking seals
Intended Location of the Meter	Indoor
Type of Register	LCD
Terminal Arrangement(s)	DIN
Location of manufacturers address	User Manual

2. Photograph of Meter and Sealing Plan

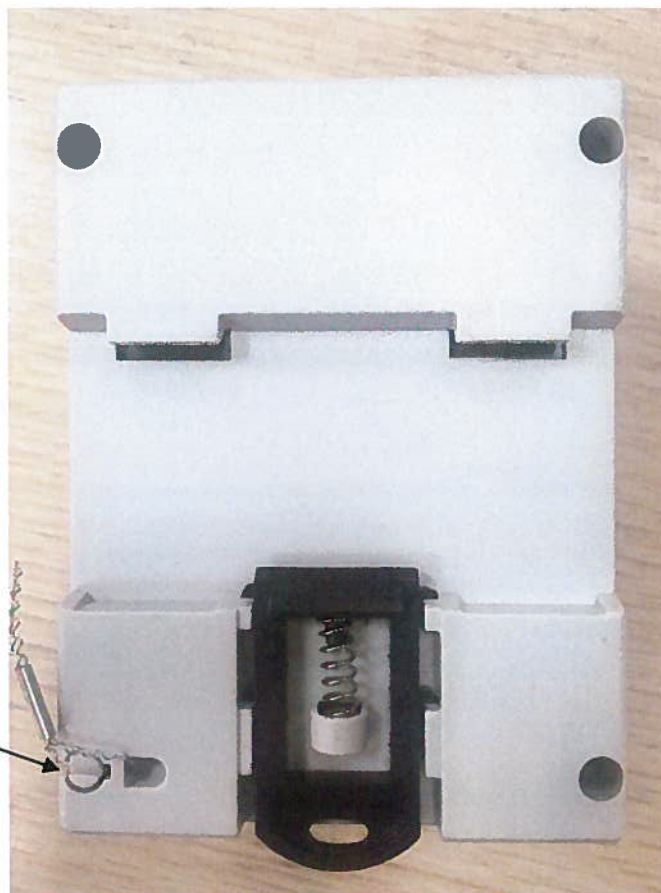

	EU-Type Examination Certificate Number:	
	0120/SGS0278	
	Issue Number: 1	Dated: 16 th May 2017

3. Examples of Nameplates

ORNO[®] **OR-WE-513** EN50470-1/3

CE **M17** **0120**

kWh

0120/SGS0278
-25°C to 55°C

3X230/400V

A
B

0,25-5(80)A

1000imp/kWh
1000imp/kvarh
S.W.1.0
50Hz

ORNO[®] **OR-WE-516** EN50470-1/3

CE **M17** **0120**

kWh

0120/SGS0278
-25°C to 55°C

3X230/400V

A
B

0,25-5(80)A

1000imp/kWh
1000imp/kvarh
S.W.1.0
50Hz

SGS

EU-Type Examination Certificate Number:

0120/SGS0278

Issue Number: 1

Dated: 16th May 2017

ORNO[®]

OR-WE-517

EN50470-1/3



CE M17 0120

  
0120/SGS0278

kWh
-25°C to 55°C
3X230/400V
0,25-5(80)A
S.W.1.0
50Hz

A 


1000imp/kWh

B 

1000imp/kvarh





	EU-Type Examination Certificate Number:	
	0120/SGS0278	
	Issue Number: 1	Dated: 16 th May 2017

4. Calculation of the composite error/ MPE


During the type approval examination the influence factors for temperature, frequency and voltage are determined per load point. The table below represents the sum of the square values per load, determined via the following formula:-

$$\delta e (T, U, f) = \sqrt{(\delta e^2 (T, I, \cos\phi) + \delta e^2 (U, I, \cos\phi) + \delta e^2 (f, I, \cos\phi))}$$

where

$\delta e(T, I, \cos\phi) =$ Additional error due to variation of the temperature at the same load
 $\delta e(U, I, \cos\phi) =$ Additional error due to variation of the voltage at the same load
 $\delta e(f, I, \cos\phi) =$ Additional error due to variation of the frequency at the same load

		Influence Factors for Temperature. Frequency & Voltage					
Current	PF Cos	-25°C	-10°C	5°C	30°C	40°C	55°C
I _{min}	1.0	0.38	0.25	0.13	0.08	0.17	0.29
I _{tr}	1.0	0.38	0.27	0.14	0.07	0.16	0.31
10I _{tr}	1.0	0.37	0.25	0.13	0.08	0.18	0.33
I _{max}	1.0	0.32	0.22	0.16	0.06	0.15	0.28
I _{tr}	0.5ind	0.38	0.27	0.13	0.06	0.14	0.31
10I _{tr}	0.5ind	0.36	0.24	0.11	0.09	0.19	0.35
I _{max}	0.5ind	0.30	0.21	0.14	0.05	0.15	0.31
I _{tr}	0.8cap	0.37	0.26	0.14	0.07	0.17	0.33
10I _{tr}	0.8cap	0.35	0.23	0.11	0.11	0.20	0.36
I _{max}	0.8cap	0.30	0.21	0.13	0.07	0.16	0.31
L1					0.00	0.00	0.00
I _{tr}	1.0	0.39	0.26	0.12	0.07	0.17	0.26
10I _{tr}	1.0	0.39	0.25	0.11	0.09	0.18	0.29
I _{max}	1.0	0.30	0.21	0.13	0.06	0.15	0.26
I _{tr}	0.5ind	0.39	0.26	0.12	0.09	0.15	0.30
10I _{tr}	0.5ind	0.38	0.25	0.11	0.10	0.19	0.33
I _{max}	0.5ind	0.30	0.21	0.13	0.06	0.15	0.28
L2							
I _{tr}	1.0	0.52	0.37	0.20	0.10	0.24	0.46
10I _{tr}	1.0	0.51	0.35	0.17	0.12	0.26	0.49
I _{max}	1.0	0.45	0.33	0.21	0.08	0.21	0.42
I _{tr}	0.5ind	0.54	0.36	0.20	0.08	0.22	0.44
10I _{tr}	0.5ind	0.51	0.35	0.17	0.11	0.25	0.47
I _{max}	0.5ind	0.47	0.34	0.22	0.08	0.20	0.41
L3							
I _{tr}	1.0	0.17	0.12	0.08	0.07	0.12	0.28
10I _{tr}	1.0	0.15	0.12	0.06	0.05	0.13	0.27
I _{max}	1.0	0.09	0.09	0.07	0.04	0.10	0.23
I _{tr}	0.5ind	0.16	0.12	0.06	0.05	0.09	0.26
10I _{tr}	0.5ind	0.12	0.11	0.06	0.08	0.13	0.28
I _{max}	0.5ind	0.06	0.08	0.02	0.05	0.11	0.24


	EU-Type Examination Certificate Number:	
	0120/SGS0278	
	Issue Number: 1	Dated: 16 th May 2017

5. Annex of Variants

Product Variant Identification Details:

Type Designation	Description of meter
OR-WE-513	3x230/400V, 0.25-5(x), energy measurement (kWh & kVarh), IR
OR-WE-516	3x230/400V, 0.25-5(x), energy measurement (kWh & kVarh), IR, RS485 (Modbus Protocol)
OR-WE-517	3x230/400V, 0.25-5(x), energy measurement (kWh & kVarh), IR, RS485 (Modbus Protocol), Multi Tariff

Modifications to the meter(s) described according to approval No. **0120/SGS0278** must be notified to the issuing body to confirm the meter(s) continuing compliance to the relevant pattern approval standard(s).

	EU-Type Examination Certificate Number:	
	0120/SGS0278	
	Issue Number: 1	Dated: 16 th May 2017

6. Document Revision History

Issue	Date	Comments
1	16/05/2017	Initial Issue

END OF TEST CERTIFICATE